

# Review on 3D printing: Fight against COVID-19

Bankole I. Oladapo <sup>a,\*</sup>, Sikiru O. Ismail <sup>b</sup>, Temitope D. Afolalu <sup>c</sup>, Francis T. Omigbodun <sup>d</sup>, Bowoto Oluwole <sup>a</sup>,  
Matthew A. Olawumi <sup>a</sup>

<sup>a</sup>*School of Engineering and Sustainable Development, De Montfort University, Leicester, UK*

<sup>b</sup>*Center for Engineering Research, School of Physics, Engineering and Computer Science, University of Hertfordshire, UK*

<sup>c</sup>*The Queen Elizabeth Hospital King's Lynn NHS Foundation Trust, UK*

<sup>d</sup>*Mechanical Engineering, Loughborough University, UK*

*\*Corresponding author, Tel: +44(0)1162013971, E-mail: [P17243433@my365.dmu.ac.uk](mailto:P17243433@my365.dmu.ac.uk)*

## Abstract

The outbreak of Coronavirus in 2019 (COVID-19) caused by the SARS-CoV-2 virus and its pandemic effects have created a demand for essential medicine equipment. To date, there are no specific, clinically effective licensed drugs and vaccines available for COVID-19. Hence, mapping out COVID-19 problems and preventing the spread with relevant technology are urgent. This work is a review of research till the middle of October 2020 on solving COVID-19 with 3D printing technology. Many patients who need to be hospitalized because of COVID-19 can only survive on bio-macromolecules antiviral respiratory assistance and other medical devices. A bio-cellular face shield with relative comfortability made of bio-macromolecules polymerized polyvinyl chloride (BPVC) and other biomaterials are produced with 3D printers. Summarily, it was evident from this review study that additive manufacturing (AM) is a proffered technology for efficient production of an improved bio-macromolecules capable of effective COVID-19 test and personal preventive equipment (PPE) to reduce the effects of COVID-19 on the world economy. Innovative AM applications can play an essential role to combat invisible killer (COVID-19) and its hydra-headed pandemic effects on humans, economics and society.

**Keywords:** Additive manufacturing/3D printing; COVID-19 pandemic; PPE; Medical devices; Health.

## Abbreviations


3D	Three-dimensional	FDA	Food and Drug Administration
ACL	Anterior cruciate ligament	FDM	Fusion deposition modelling
AM	Additive manufacturing	HP	Hewlett-packard
AP-HP	Paris public hospital assistance	NHS	National health service
CAD	Computer aided design	NP	Nasopharyngeal
CDCP	Centre for disease control and prevention	PETG	Polyethylene terephthalate glycol
CHU	Centre hospitalier universitaire	PPE	Personal preventive equipment
COVID-19	Corona virus in 2019	PVC	Poly vinyl chloride

DLP	Digital light processing	SLA	Stereolithography
ECG	Electrocardiogram	TI	Texas instruments
EPP	Erythropoietic protoporphyria	USF	University of South Florida
ETH	Eidgenössische technische hochschule	VR	Virtual reality

## 1. Introduction

In recent months, severe acute respiratory syndrome coronavirus (COVID-19) has continued to spread worldwide at an alarming rate, regardless of pre-existing medical conditions, age, or other patient demographics [1-3]. The death rate is significantly higher than that of the flu, and the death rate in the United States gives the impression to be higher than in China and Europe. Every morning and afternoon, their degree of illness, their health, and safety are threatened [4-6]. The medical community has experienced a worrying reality: there is a complete lack of resources for patients and caregivers. In particular, personal protective equipment (PPE) has a critically low supply power. Consequently, it puts both patients and caregivers at unacceptable risk.

During a severe outbreak of fatal acute respiratory syndrome of the Coronavirus in the following year 2020, healthcare professionals blamed 21% of cases for an alarming situation, a trend that should be avoided. Many people and companies have implemented different strategies to meet or respond to these needs [7-9]. Improvisation without the necessary equipment to protect healthcare professionals will lead to not only a significant deterioration in hospital affairs and inaccessible pressures in the supply chain but also a severe risk to the lives of those who seek healthcare rest of society. The spread of COVID-19 is mediated by different droplet contacts and direct exposure to air. Different levels of protection are necessary for various procedures and interactions between patients [10,11]. For any healthcare professional, there is always at least one suspected patient or proven infection. Therefore, wearing PPE such as overall clothing, gloves, some antibacterial bio-cellulose masks, and eye/face protection mask is an unavoidable practice [12-14] (Fig. 1). The universal ideologies governing the biological evaluation of medical devices within a risk management process are recognition of extra data sets essential to analyses the biological protection of the medical device of the valuation of the biological protection of the medical device. This research is applicable to biological evaluation of all types of medical devices, including active and non-active. In this research, assessment of biological hazards arising from risks, such as variations to the medical device over time, as a part of the overall biological safety assessment is important and described explicitly. To comprehend how this transpires, it is essential to distinguish the unique structure of different masks and PPE as well as understand their biomolecules that could cause their structures modified, due to the action of a given chemical agent and, thus, lose their biological action capacity.

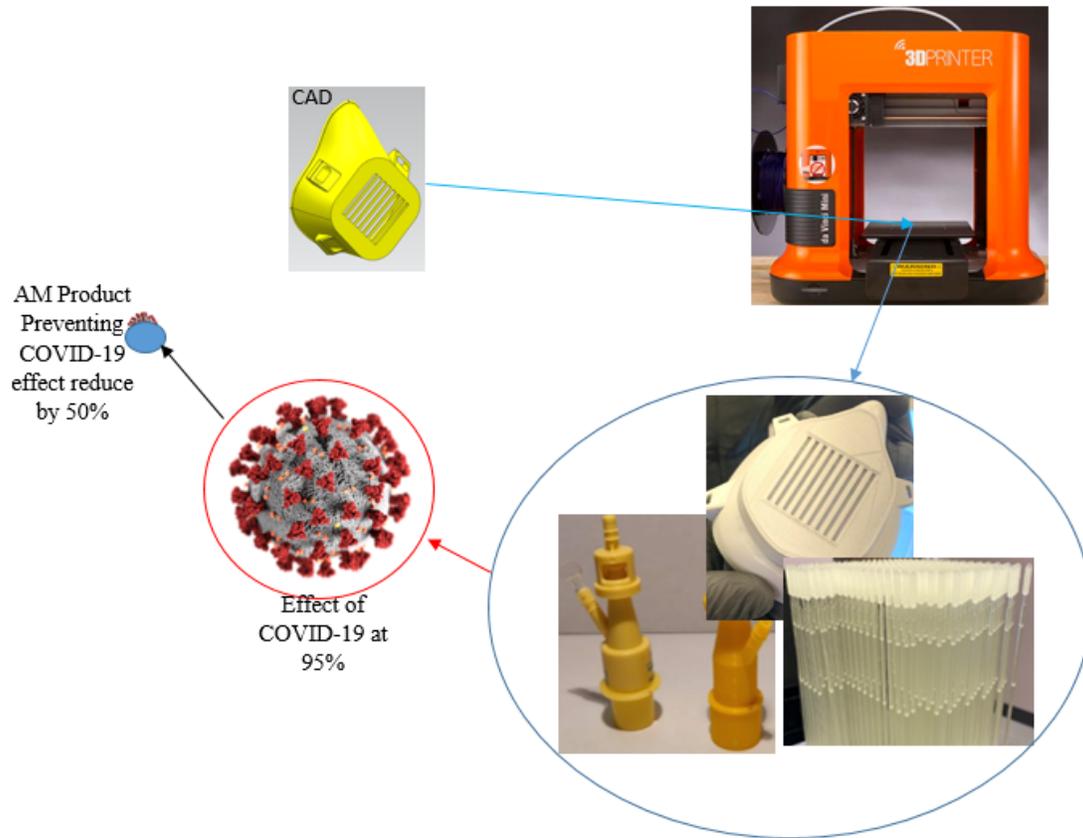

**Fig. 1.** Step description of the effect of additive manufacturing (AM) on COVID-19.

Furthermore, to perform the COVID-19 tests, healthcare workers need nasopharyngeal (NP) antibacterial bio-cellulose swabs, small flexible rods to insert into a patient’s nose to take samples made of biomaterials. Once the sample has been taken, they are stored in a bottle containing a culture medium. These antibacterial bio-cellulose swabs are very necessary for today’s medical sector, which faces a severe shortage of equipment to fight the virus [15-17]. It has been demonstrated in many ways, such as the use of a three-dimensional (3D) printing initiative, to avoid the shortage of resources. To offer solutions to this situation, there are Carbon, Formlabs, and two resin 3D printer manufacturers, who produce thousands of antibacterial bio-cellulose swabs every day [18-20]. Some researchers [20-22] had effectively manipulated 3D printing technology to help health care workers on the front line of the COVID-19 anti-epidemic and make antibacterial bio-cellulose masks from biocomposite materials. The extraordinary period requires extraordinary measures, as stated by a packaging engineering manager in Malaysia [21-23]. Initial programming with a 3D-printed antiviral bio-cellulose masks design online was started and proposed using TI’s production site in Kuala Lumpur for production. A faster, easier-to-assemble scheme that cuts print time to half was developed. Three days later, the prototype was made. It is essential to provide a more efficient product design. It was followed by printing about 20 masks made of antibacterial bio-cellulose masks in a day and delivered them to

public health care providers every week. The shortage of medical supplies is increasing as the COVID-19 pandemic strains global supply chains. Malaysia team is using 3D printing technology to manufacture medical devices and supplies worldwide, including medical devices such as bio-cellulose swabs, antibacterial bio-cellulose masks, and test boxes [24-26]. According to Fig. 2, the highest number of cases from the World Health Organization as at September 14, 2020 is in American continent and the lowest occurs in Africa and some other Asian countries. There are countries without any reported new case, according to the figure. This is a 14-day COVID-19 case notification rate per 100,000. American continent recorded above 120,000 out of the total confirmed number of COVID-19 cases and how rapidly they increase in American continent. The number of confirmed COVID-19 cases is lower than the number of total cases. This is due to limited materials for testing, such as PPE to protect the sample collector/health workers and swab for testing.


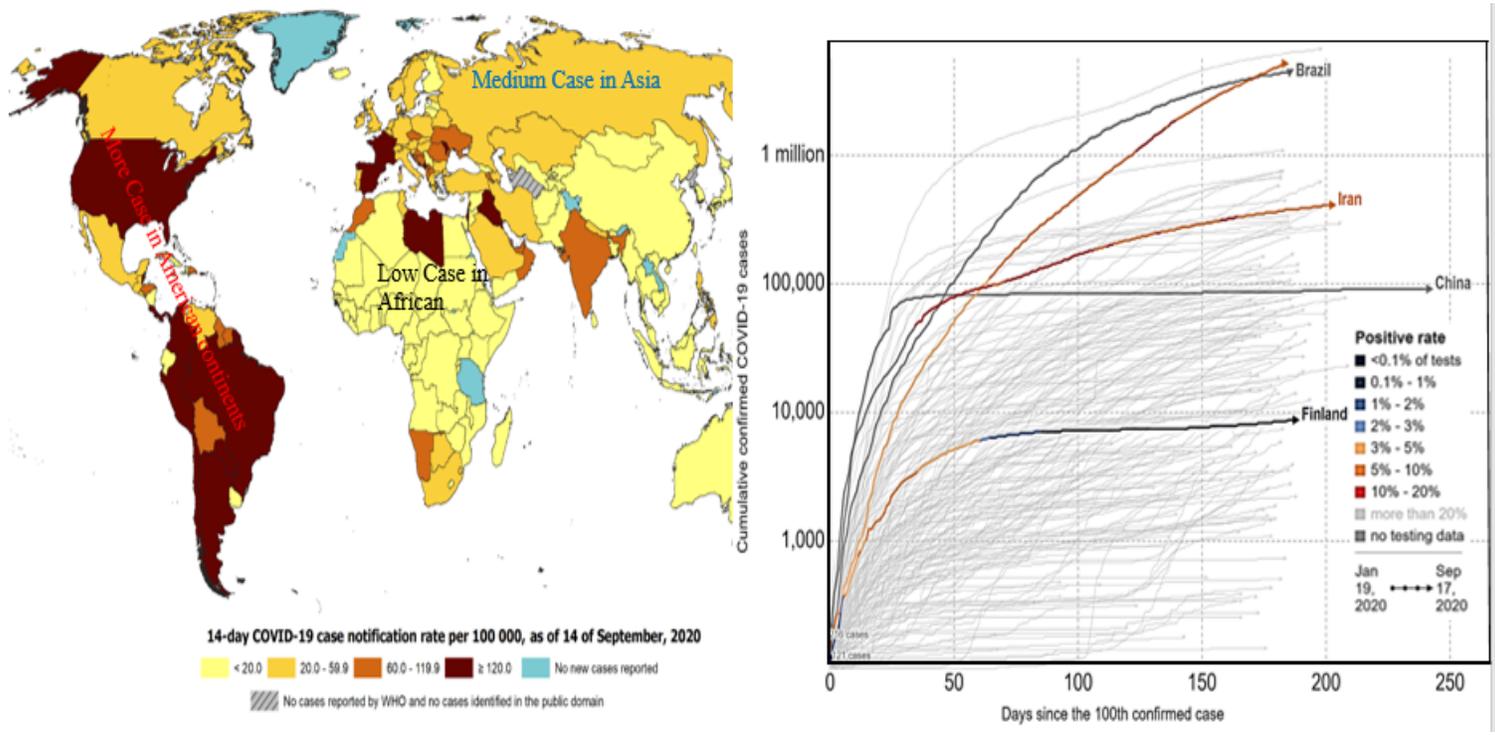


Fig. 2. Geographic distribution of cumulative number of confirmed COVID-19 cases per one hundred population, worldwide, as of September 14, 2020 for 14-day interval [24,25].

After connecting to compressed air or oxygen at a rate of 15 L/min, air flows through the hood and prevents the supplier from inhaling the patient’s aerosol kit. It is essential to emphasize. One of the additional gas flow is not used with the face protection configuration, a venturi effect can be created, and the atomized particles can be transported to the supplier’s face. This PPE is not designed to be used in Place of robust air purification systems capable of producing more than 100 liters per min. To avoid hypercapnia, it should be used for a short period with a different mask of bio-cellulose materials on the hood [27-29]. Fig. 3 represents the schematic process of the need for design and 3D printing of PPE to tackles the shortage of medical device during COVID-19 pandemic. This process in taken serious, because of the increasing number of confirmed death of COVID-19 patients per day data, especially in the highest effected country from the first day with over 100 cumulative death from world meters of National Health Agency.

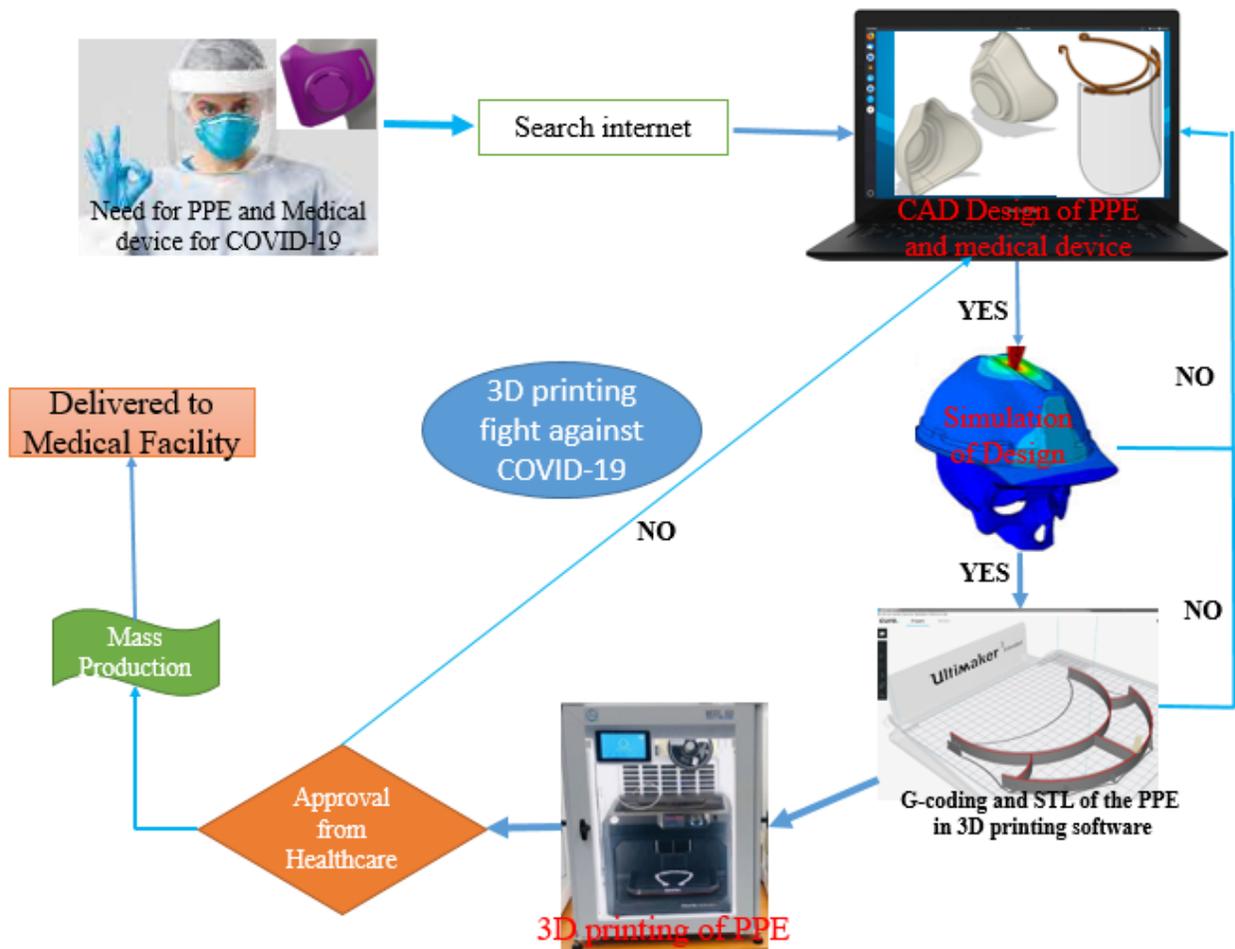

**Fig. 3.** Schematic process of the need, design and 3D printing of PPE to tackle the shortage of medical device during COVID-19 pandemic.

### 1.1. *Brief evolution of 3D printing*

The evolution of medical 3D printing over the past decade has followed imagination and problem-solving ways. Starting as a novelty with limited practical value, 3D printing has grown to find primary uses and acceptances in various industries, including engineering, car manufacturing, military manufacturing, and healthcare. Although the variety of these paths is impressive, it requires to combine efforts to satisfy a collective need. The concentrated efforts of 3D printing enthusiasts and 3D printing laboratories can address the critical deficiency of PPE during the global COVID-19 outbreak. This research aim at reviewing the role of 3D printing, especially in the production of face shields, to examine feasibility and engagement under the new CDCP and FDA pandemic guidelines, and to propose a concentrated effort towards improvement of the 3D printing industries [30-32], as depicted in Fig. 4.




**Fig. 4.** The different 3D-printed respiratory antibacterial bio-cellulose masks that allow inflow and out of oxygen during COVID-19: (a) oxygen inflow for respiration, (b) nose and eyes biomaterial mask, (c,d) respiratory mask with eye, (e) micropore nose antibacterial bio-cellulose mask and (f) lateral nose mask.

## **1.2. *Relevance of 3D printing to the medical profession***

Therefore, with these new and comfortable guidelines, 3D-printed face shields have a clear role to play. Support and encouragement must be continued efforts across the country. Professional companies, such as Prusa Research, based in the Czech Republic, began sharing open-source mask designs and allowed anyone with a 3D printer to download and use the free plan. The family that buys 3D home printers can now remove several hundred face shields in a week. On a larger scale, 3D printing manufacturers are also transforming their efforts to produce face shields and other PPE. In particular, the military and automotive industries include news organizations reporting joint efforts to work together in the military, consolidate resources, and determine the scope and volume of 3D printing resources [33-35]. Ford Motor Company has facilities that operate on 3D-printed PPE, including a facility that produces approximately 1,000,000 face shields per week in Plymouth, United Kingdom [36-38]. 3D printing factories have machines that support wireless connectivity and sensors. These sensors are connected to a system that can view and monitor the entire production line and make its own decisions. 3D printing uses smart manufacturing processes to manufacture primary disposable products to solve the COVID-19 outbreak deficiency[39-41]. During this crisis, it provides a supply chain and intelligent disposable medical supplies of equipment, where patients can obtain essential medical supplies on time. In this comprehensive review, the applications and benefits of 3D printing technologies to manage the COVID-19 outbreak have been subsequently considered.

## **2. *Oustanding benefits of 3D printing for COVID-19***


Additive manufacturing technology has the capability of providing better digital solutions for daily lives during this crisis. More also, digital technologies include, but are not limited to, virtual reality, holography, 3D scanning, 3D printing, and biosensing. These modern technologies support effective methods of printing of several and specially designed PPE that are relevant to combat COVID-19 pandemic, with less stress, time and material usage. The effects of limited testing and challenges in the attribution of death means before the use of masks and lockdown as well as after the introduction of mask are represented in Fig. 5. The death rate was controlled by some highly affected countries: China, UK and Iran, because of the quick intervention of lock down and face mask to control the spread of the invisible killer. The 3D printing of different PPE helped to meet the demand. While some affected countries still experienced some lost, due to their slow intervention. But for many countries, the spread was minima due to the introduction of use of PPE, which can be majorly attributed to 3D printing materials. The information presented in Fig. 5 is the latest data from the Our world in Data as at September 14, 2020, from the European update worldwide from January 21 to September 14, 2020.

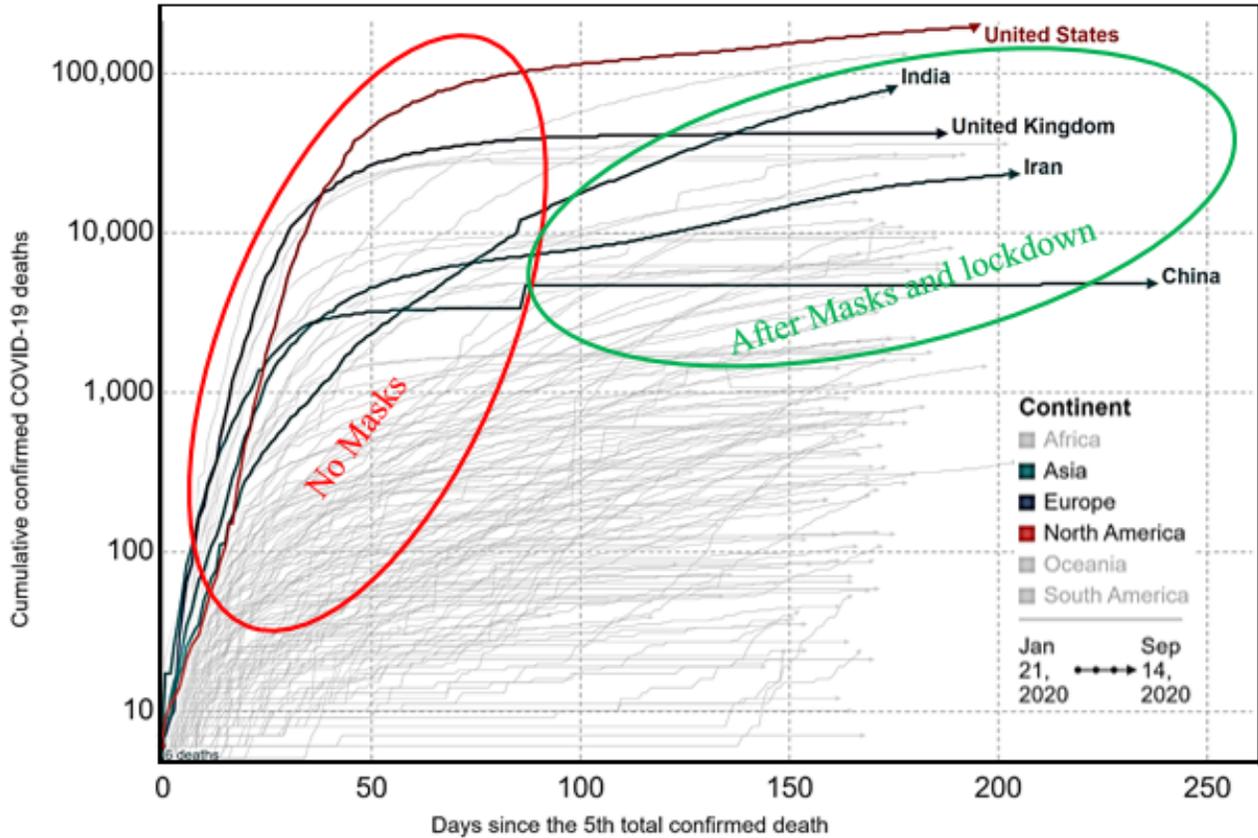

**Fig. 5.** Cumulative number of confirmed deaths *versus* number of days in continents, modified from Our World in Data chart points to establish the importance of use of face masks and lock down mechanism [66].

### 2.1. 3D antibacterial bio-cellulose swabs lattice structure for COVID-19 test

As earlier mentioned, the Manufacturer Volumic has thousands of 3D-printed test tubes validated by the competent laboratories to detect the virus. This is good news for the health sector, which can rely on this type of solution and technology in emergencies. Volumic 3D prints the test tubes needed to screen for COVID-19. Further south, on the Nice side, Cerballiance, Volumic, and LaFerme3D Laboratories have joined forces to produce COVID-19 testing tools, using 3D printing. In 3 days, a solution to the problem posed by the Cerballiance laboratory was provided, as explained by Stéphane Malaussena, co-founder of Volumic 3D. As of today, there are thousands of test tubes printed in France daily in an attempt to expedite COVID-19 screenings. Cerballiance, an initiator of the project, shipped the test tubes produced in Nice to its various laboratories on the territory (600 in France), but also to its conferees who need the equipment [42-45]. The Volumic’s boss stated that they continue to produce to date, since there is no instruction to stop production (Fig. 6).

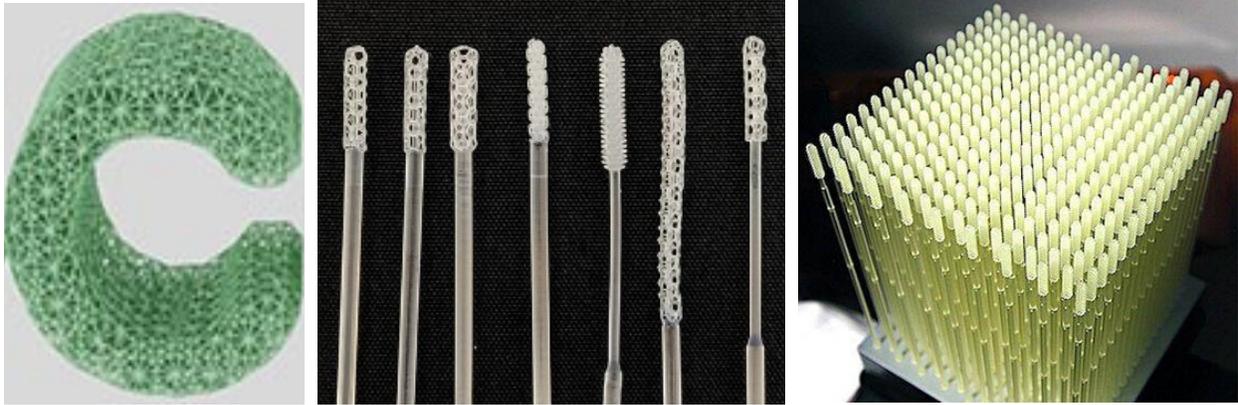

**Fig. 6.** Lattice structures of the 3D-printed antibacterial bio-cellulose swabs produced for the COVID-19 test.

Furthermore, printing glass objects is now possible, and the most common method involves either extruding melted glass, or selective sintering laser heating ceramic powder, which is converted into glass. The former requires high temperatures and therefore requires heat-resistant equipment, while the latter cannot produce particularly complex objects. ETH's new technology aims to improve these two disadvantages. It contains a photosensitive resin consisting of liquid plastics and organic macromolecules that bond with silicon-containing macromolecules, in other words, ceramic macromolecules. Using an existing process called digital light treatment, the resin is exposed to the pattern of UV light. Plastic monomers are cross-linked to form solid polymers wherever the light hits the resin. The polymer has a maze-like internal structure, and the space inside the maze is filled with ceramic macromolecules [46-48]. The resulting 3D object is then burned at a temperature of 600°C, burning the polymer, leaving only the ceramic. In the second roasting, the roasting temperature is about 1000°C, and the ceramic is compacted into the transparent porous glass. The object does shrink significantly when converted to glass, which is a factor that must be taken into account in the design process. Although the objects created so far are small, the shapes are somewhat complicated, as reported. Also, the aperture can be adjusted by changing the UV intensity, or other properties of the glass can be altered by mixing borate or phosphate into the resin. A major Swiss glassware distributor has expressed interest in using the technology, which is similar to the equipment developed by the Karlsruhe Institute of Technology in Germany [49-51], as shown in Fig. 7.




**Fig. 7.** 3D printing of respiratory face shield using double-sided tape, showing the (a) CAD design, (b) printing process, (c) finish product and (d) complete face shield with films.

## 2.2. *3D-printed antibacterial bio-cellulose masks and respirator valves*

COVID-19 ravaged Italy. Despite the medical system in the country, Italy was overwhelmed. According to the latest statistics on March 19 2020, Italy recorded 3405 deaths from the outbreak. The data for the first time was more than the total death outbreaks recorded in China. To save Italy, the European 3D printing industry moved to solve the urgent problem through open masks but of antibacterial bio-cellulose materials, small door-to-door objects of 3D printing design files, and helped in a rush to print respirator valves [52-54]. The outbreak of pneumonia in Wuhan, Italy was out of control; the number of confirmed explosion struck and collapsed the medical system. To help the first line of medical care to share the pressure, the European technology industry has to move in and assist them. The first

is in the mask section, although the antibacterial bio-cellulose mask is one of the most important instruments for the public to fight the virus. Still, because the outbreak was snapped up, Italy's 3D printing industry brain-headed, launched a *Pugliese-Sicilian* open original code [55-57].

The team behind the programme, which builds a web platform that allows users to freely download mask design files to print antibacterial bio-cellulose masks at home with 3D printing devices, as reported by their programme's leaders. They built a platform that everyone can adapt, improve, and spread, and hope to find other applications in the future, in addition to fighting viruses. Also, 250 patients with coronavirus were in intensive care at a hospital in Brescia, Italy. Still, they all needed respirators, which were in short supply and must be replaced for up to eight hours each, but suppliers have suddenly burst into supply, because of market demand [58-60]. At this point, Cristian Fracassi, chief executive of Isinnova, an Italian 3D printing manufacturer, decided to come forward and, within three hours of studying the valve, returned to the hospital with a 3D-printed respirator valve prototype (Fig. 8a) to test the patient. When they found out that the valves made out of 3D printing could work, they immediately returned to the Company to start a large number of printing, quickly put into production, and in just one day, it took a day to design and print 100 respirator valves for a hospital, successfully solving the shortage of hospital medical equipment [61-64].

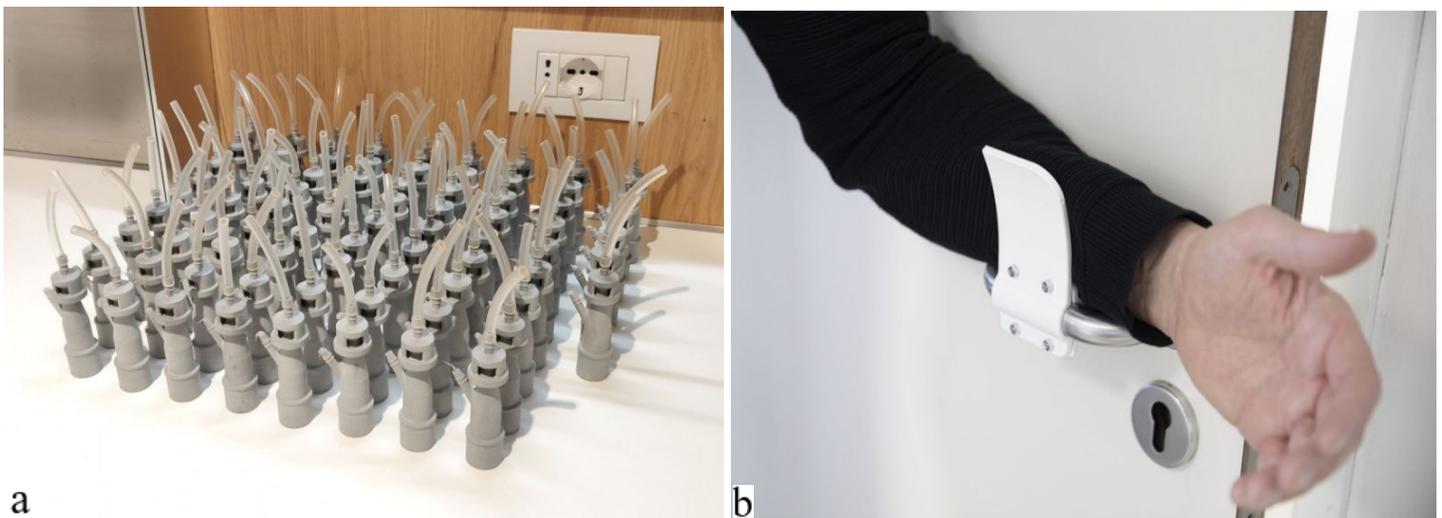

**Fig. 8.** A respirator valve made of 3D printing, showing (a) 3D-printed respirator valve prototype and (b) materialized, designed and 3D-printed door opener.

### 3. The development of respirators through 3D printing

Central News Agency reporter Dai Yazhen London 24 thumped by Wuhan pneumonia, the demand for respirators increased, cross-cutting team to develop rapid deployment, and production of respirators is now entering the clinical testing stage. The cross-disciplinary team, led by engineers, anesthesiologists, and surgeons, is aiming to

develop a production model for breathing equipment that meets safety and stability needs and uses off-the-shelf components to increase the capacity of respirators in the UK [65-67].

Research of Oxford University's School of Engineering says the time of crisis or pandemic requires extraordinary responses. They assembled an excellent team with endless creativity and outstanding skill levels, using their experience to transform existing research results into devices that can be used in medicine. The team is building and testing a new respirator prototype that can be produced by universities with equipment, as well as small and medium-sized businesses, to address the massive demand for respirators in the UK in the face of the invisible killer (COVID-19) outbreak (Fig. 8). The team said that by developing an open-source design that meets security and stability needs and complies with local laws and regulations, it would be able to achieve significant capacity potential through decentralized production. Under government regulation and market competition, better models will be developed, universities, small and medium-sized enterprises, and factories will be able to produce from existing equipment, assemble local medical facilities, and adjust capacity to local needs, thereby reducing the pressure on the National Health Service (NHS) to allocate medical resources [68-70]. Farmery, a professor at the School of Clinical Neurosciences at The University of Oxford's Nuffield and Wadham states that medical equipment development usually takes several years and is an extensive project. But, they designed a simple and reliable breathing device to meet the needs of critically endangered patients during an outbreak with the collaboration of experts, the open-source design, and the fast approval process. They are pleased to be able to take such a rapid step into this outbreak. Not only do, but they also have to share their experiences with countries that don't yet have the resources to have a ready-made respirator, and they are constantly improving this relatively low-cost technology. A researcher from the Oxford University School of Medical Engineering in Taiwan assisted in mechanical design, 3D modeling, and printing in this project (OxVent). He studied biomechanics, bone dynamics, gait analysis, 3D printing, and modeling, and has served as President of the Robotics and 3D Printing Society at Oxford University [30,31,71-74], as depicted in Fig. 9.




**Fig. 9.** 3D-printed ventilator and respiratory system in Oxford University [30-33].

Mr. Zhan appreciated the 3D printing technology for reducing the time it takes to manufacture and test prototypes. And 3D-printed components can be distributed and produced rapidly around the world, helping countries with scarce medical resources. They are developing day and night in the hope of contributing to the outbreak of pneumonia. The UK is hit by new coronary pneumonia, and demand for respirators has increased, with Oxford University and a cross-cutting team at King's College London developing rapidly deployable and produced respirators that are now in clinical testing.

#### **4. Shortage of medical supplies: Rescue through 3D printing**

Under the outbreak of new COVID-19 pneumonia, some local medical supplies are in short supply, 3D printing technology is widely available, print protective antibacterial bio-cellulose masks, among others. It helps to ease the tension of materials. There are also some 3D printing epidemic prevention supplies. The UK has set up its online platform 3D Crowd UK to recruit volunteers to work on 3D-printed antibacterial bio-cellulose masks, and as of Friday, April 10, 2020, the website received requests from local health care for 500,000 3D-printed antibacterial bio-cellulose masks, bringing together more than 6,000 volunteers as of preceding Monday. A software engineer in Hertfordshire, England, responded to the call by using two 3D-printed macromolecular mechanisms to remove 150 masks from his home and gave 39 of them to local nurses and midwives. Maker Nexus, a California-based non-profit organization, uses 13 3D printers and three laser cutters to make 1,800 protective antibacterial bio-cellulose masks for local hospitals, and General Manager Eric Hess says 300 volunteers help search the web for raw materials for making. In daily life, the door attendant is less necessary to touch the door handle. Still, the door handle is easy to become a virus temperature, Belgian Company materializes a screw-free hand door opener, as previously shown in Fig. 8(b), made

with 3D printer within 4 hours, only 3 ropes can be fixed in the door handle, with arm down to open the door, without touching the door handle. Hence, it reduces the risk of infection [76-79]. Fig. 10 represents the operation *The Visières of Hope*. It was initiated by 3D natives, mobilizes industrialists, such as L'Oréal, Schneider Electric, Renault, Faurecia to mass produce visors for hospital staff.

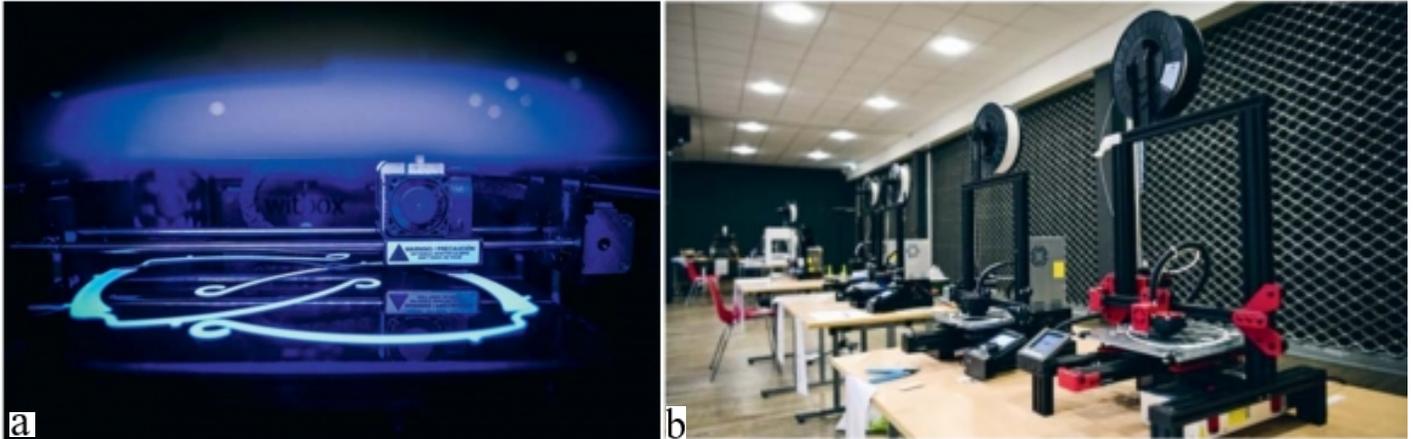

**Fig. 10.** The operation *The Visières of Hope*, initiated by 3D natives, mobilizes industrialists, such as L'Oréal, Schneider Electric, Renault, Faurecia to mass produce visors for hospital staff.

In addition, 3D-printed circuit splitter and flow restriction devices for multiple patient lung ventilation and Prusa protective face shield - RC2 have been invented. The makers are involved in the fight against the pandemic, such as the collective La Fabrik-Ephémère, where some forty passionate handymen make up to 600 visors a day in a space made available by the municipality. Initiatives of this kind are multiplying [80-82]. The University of Nantes (Loire-Atlantique) has teamed up with the *Centre Hospitalier Universitaire* (CHU) and the industrial Armor to design protective visors. At least 800 were delivered to the hospital. Each is designed with polyethylene terephthalate glycol (PETG), or glycolysis polyester, to which is added a supporting elastic and a headband produced by Armor. The whole device is assembled in The West Hall 6 on the island of Nantes. In the Yvelines, the Renault group has mobilized its Flins site and the Technocentre in Guyancourt, with the aim of printing 2,000 visors for the André Mignot hospital in Chesnay-Rocquencourt [83-85].

#### **4.1 Involvement of other non-medical manufacturing companies**

In this race against time to equip caregivers, machine manufacturers have made all their capabilities available. The American Hewlett-Packard (HP) Company has published in open source five digital plans validated and adapted to its machines. Its emergency catalog ranges from the *elbow handle* for doors to protective visors. Nicolas Aubert, director of 3D printing at HP France, argues that they are reaching relatively large production volumes. This is the

advantage of an industrial system. HP's machines, such as those of fellow Stratasys, use powder bed fusion technology rather than wire-depositing technology from desktop printers [86-88]. They can produce several parts at the same time: in a single print, an HP machine produces 70 visors simultaneously, in 24 hours. And the parts are stronger, resistant in particular to high-temperature sterilization in an autoclave, which makes them reusable. Another advantage is that production is relocated to customers. Jos Burger, CEO of desktop printer brand Ultimaker reported that they connected more than 4,000 printers worldwide in less than a week to Universities, designers, makers, engineers, among others. It has a whole network that is coming together[89-91]. HP mobilized its L'Oréal and Decathlon customers, and Stratasys formed a coalition of more than 150 companies, including Boeing, Toyota, and Medtronic. It is the brands that link the requests of the hospitals to different points of production. They also connect with design experts, biocompatibility, and designers. This is enough to create an entire ecosystem of open innovation, involved in an unprecedented mobilization [92-94].

## **5. Progress of 3D printing in Medical**

### **5.1. 3D-printed medicals**

Just over a year ago, some medical practitioners were worried that advances in 3D printing would put them out of work. Medicine is one of the fields that will have a revolutionary impact on 3D printing. In contrast, repair doctors and other medical practitioners are worried that traditional industries that were otherwise "calm" have been invaded by the new 3D printing technology [94-96]. According to the research firm, Industry Arc, the global 3D printing market will reach \$1.2 billion by 2020 [96-98]. It is a technology that uses a digital object created in the software, with melted plastic or metal powder, superimposed on layers on a 3D scale. 3D printing technology existed as early as the 1980s. However, 3D printers, priced between \$2,000 and \$8,000 and small enough to be on a table, have only begun to appear in the last decade. The latest medical applications of 3D printing started a few decades ago. In 2016, 3D printing continued to thrive in the healthcare industry. The world's first 3D-printed prescription drug, Spritam, was approved by the US FDA in March 2020, it has gone on sale. 3D-printed medical devices now cover surgical instruments and human implants, such as certified Medical Shape titanium bone connecting plates [98-100].

Institutions, such as Boston Children's Hospital, are also increasingly using 3D-printed organ and bone models to plan and practice complex surgeries. Earlier this year, the Department of Neurosurgery at the University of St. Louis and the St. Louis School of Engineering jointly designed a highly simulated, 3D-printed brain aneurysm [99-101]. Stratasys, one of the world's largest manufacturers of desktop and industrial 3D printers, produced the final model. All aneurysms are different in size, contour and position, as reported by Saleem Abdulrauf, director of neurosurgery at St. Louis University Hospital. There are hundreds of different sizes and types of surgical clips. The decisions on which one to choose are made during surgery. He said that practice on the model in advance and choose a good surgical clip model can really improve the procedure, after simulating surgery on a 3D-printed aneurysm model [100-102].

## **5.2 Prosthetics, 3D-printed trachea splints and Stratasys brain model for surgical simulation**

Analysts have predicted that 3D printing will be a disruptive force in the healthcare industry by 2020. According to research by Gartner Study, one in ten people in developed countries will have 3D printing devices physically or in the body by 2019. Also, about one-third of remediation and implant surgery will use 3D printing as a core tool [101-103]. Prosthetics are a good example, it shows how 3D printing can improve people's lives. Typically, the process of making a prosthesis involves measuring the size of the rest of the limb, making a plastic replica and then hand-out the specification improvement score. Standard Cyborg, a San Francisco-based start-up, sells 3D scanners and software that allow customers to make prosthetics, modify shapes and print them out. The result is a fully functional prosthesis that is made available in a short time. In contrast, traditional methods of making prosthetics take four hours [66-69].

Lei Feng stated that, at first, practitioners considered 3D printing as a threat. Now, Jeff Huber, co-founder of Standard Cyborg, said that his clients and the repair doctors are more likely to introduce 3D printing and design into clinical applications [68-70]. The main reason for the shift is that 3D printing allows experts to create complex geometric shapes to ensure a precise fit. Machines are not intimidated by complexity, and for patients, a more refined design delivers superior comfort. 3D printing also allows surgeons to treat patients with the help of a copy of the human anatomy. Researchers at the University of Michigan, for example, worked with surgeons at C.S. Mott Children's Hospital to develop 3D-printed trachea splints that were implanted into five children with congenital bronchitis. Developers are applying for special FDA permission to treat more patients [68-71], as the quest to improve health care continues.

## **5.3 Ethical considerations for AM/3D-printed PPE for COVID-19 and other related medical applications**

It is evident that AM/3D printing technology has wide applications in biomedical engineering. It has been well integrated into the medicine and pharmaceuticals for organ/tissue bio-printing and drug delivery, respectively [104]. This is attributed to its capability to provide patient-specific design, on-demand and cost-effective printing, high productivity and complexity, to mention but a few [105]. Presently, AM/3D printing technology has been effectively used to print various PPE to combat the invisible killer (COVID-19). The design conceptual stage of PPE, creation of low-price and customized precise anatomic prostheses (such as lower limbs, hands and arms) and orthoses (foot, ankle-foot and wrist splints) [105], among other artificial body parts utilized in various medical applications. The use of the aforementioned 3D-printed medical safety devices/PPE, patient-specific prostheses as well as orthoses required careful ethical considerations and approval by the authorized medical/health organizations.

Ethical issue includes whether AM products meet the stringent medical requirements, especially in view of the potential for AM to be employed for long term COVID-19 and other related medical applications. For example, there is an ethical concern (challenge) with the 3D printing of PPE against COVID-19. This include reaction of PPE material

with other substances: water, sweat, chemicals, such as different types of sanitisers, among other medical sterilization materials, with human body parts (especially face/head and hand). Care must be taken to ensure that none of these materials has health risk or hazardous effect on the users. Also, the cost of PPE should be affordable to avoid widen the gap between the rich and poor. Both the 3D printing process and product tests are very germane for the sake of human safety. Importantly, the government has started regulating the workflow associated with 3D printing in medicine by weighing the benefits and disadvantages of this innovative and revolutionary technology. This involves prevention of possibility of making unprofessional and destructive changes to the digital file when creating an organ, after hacking into the 3D printers. The concern is that how will this injurious act be known earlier than the time that the 3D-printed organ started displaying trouble, shortly after transplant and when it is in full use [106]. The principal ethical consideration in device regulation is to avoid acceptance of a high level of risk during the market approval stage. Hence, both pre-market and post-market studies, investigation or compliance must be enforced [108] to protect health care providers and patients.

Furthermore, the cost of 3D printing-assisted treatment offer to the patient is a serious ethical issue. This may not be affordable or inexpensive if the medical application of 3D printing is left in the hand of the private health care sector. It is worth remembering that one of main goals of private company is to maximize profits. Also, there is an anticipated long procedure and/or time before patient can benefit. Therefore, patients may decide to pay more in order to get the service. This may lead to crime through organ smuggling. It is an ethical measure for the government to regulate the cost of 3D printing-assisted treatment. In addition, it may end up becoming a technology for the wealthy people only. What will be the hope of the poor? If measures are not properly taken, there may be repetition of the past with 3D printing technology; whereby there was a wide discrepancy between the poor and rich in terms of medical treatments. Though, 3D printing is already in the customer-use domain, but 3D printers designed for medical applications are insufficient [106].

Close to this point is to know the efficient method to test the 3D printing-assisted treatment. Foremost, the safety of the treatment must be guaranteed before the treatment is made available for the patients. It is expected and mandatory that all the human or *in-vivo* tests must be accurately conducted and the results obtained must be 100% satisfactory. Moving forward, the usage of the 3D printing-assisted medical treatment must be stringently regulated. This should involve numerous applications of 3D printing in the medical sector, including for both essential and personal enhancements, such as cosmetic surgeries. The essential medical treatment should be regulated, while the non-crucial counterparts are ignored. To identify the differences between the two may be a challenge, because it depends on individual interest. The government can help to find the difference and make decisive regulations [106]. These regulations include design control (21CFR820.30), purchasing controls (21CFR820.50), traceability (21CFR820.65), production and process control (21CFR820.70), process validation (21CFR820.75) as well as acceptance activities (21CFR820.80), among others [107]. Introduction of new and manageable regulatory considerations are expected from new processes, materials and value chains of 3D printing technology [107].

Moreover, present ethical challenges of using 3D printing technology for medical purposes include, but are not limited to, availability, acceptance and approval of some AM processes and volunteers for *in-vivo* tests. Also, absence of recent international regulatory directives to guide these tests is a part of the limitations [109]. For instance, there is no developed 3D bio-printing strategy by European Union, despite of commercialization of numerous applications of 3D bio-printing. However, these drawbacks are not insurmountable, as there is an increasing in the number of people who are making themselves available voluntarily for COVID-19 drug trial tests recently. Also, support and ethical approval from medical organizations are increasing. However, some American companies hesitate to adopt 3D printing technology, because of the complexity of US FDA regulations and requirement of long days for approval [107,108]. In addition, there are some ethical dilemmas from xenotransplantation (a cross-species transplantation, especially from animal/human to human). When it is between humans, it is unethical if the donor is not well informed of either current or future use (or both) of his/her cells and tissues. Therefore, a consent form is needed to contain full details of the bio-printed part composition, implantation procedure, all possible results, all conflicts of interest as well as prospective adverse effects [110].

Summarily, in a bid to maximize the potentials of 3D printing to fight COVID-19 in addition to other related medical applications, it must be well regulated by carefully bearing in mind all the probable related ethical issues. Now, can mutated organs be 3D-printed for a healthier lifestyle and consequently a longer life span, probably to live for 15 decades on earth? [106]. The bright and promising future of 3D printing-assisted medical treatment has the answer to give.

## 6. Concluding remarks

A comprehensive evaluation of relevant biological safety endpoints in compliance with relevant ethical regulatory directives and safety standards, such as the biological safety standards series ISO 10993 for antibacterial bio-cellulose masks and ventilator, is essential. Any vapors, wear debris, degradation products and processing residues that may be released from the 3D-printed part must be non-toxic to a high level of assurance. The respiratory illness due to the COVID-19 pandemic can be reduced and may be stopped eventually with the use of AM technology. The steps involved in the supply chain management of ventilators must be increased with AM to produce more PPE to prevent the spread of COVID-19. The 3D-printed face shield is well accepted in several interventions. 3D printing provides an automated solution for various manufacturing industries and other related fields for the production of medical equipment during the COVID-19 crisis. AM technologies provide an innovative method to adequately isolate the infected patient to reduce the risk of high mortality. With the application of 3D printing technologies, efficient production of PPE and other medical equipment is possible. 3D printing can work remotely with smart technologies that are useful for monitoring and prevention of COVID-19 spread. In any environment with a high oxygen atmosphere, fire risk is certainly a concern and should be discussed and mitigated. In the authors' opinion, during the

COVID-19 pandemic, all the aforementioned risks are outweighed by the benefits of protecting healthcare professionals and enhancing patient safety during this global crisis, using innovative and revolutionary 3D printing technology. As a respiratory disease, due to the COVID-19 pandemic spreads across the world, healthcare systems and national governments face difficult challenges of getting ventilators to help several patients. AM/3D printing technology can ensure that antibacterial bio-cellulose masks and ventilators, among other equipment, get to patients and prepare us better for such viral outbreaks in the future, probably and undesirably in the next ten decades.

### **Ethical statement**

The authors declare that there is no ethical issue; the study was conducted in full agreement with ethical standards.

### **Declaration of competing interest**

We hereby affirm that there is no conflict of interest.

### **Acknowledgment**

We appreciate the funding/financial support received from the Higher Education Innovation Fund (HEIF) of De Montfort University, Leicester, United Kingdom, under Research Project No.0043.06.

### **References**

- [1] M.M. Erickson, E.S. Richardson, N.M. Hernandez, D.W. Bobbert, P. Fearis, Helmet modification to PPE with 3D printing during the COVID-19 pandemic at Duke University Medical Center: A novel technique, *J Arthroplas* In press, corrected proof Available online April 18 2020.
- [2] C.R. MacIntyre, Global spread of COVID-19 and pandemic potential. *Global Biosecur* (2020) 1.
- [3] J. Yee, L. Unger, F. Zdravec, et al., Novel coronavirus 2019 (COVID-19): Emergence and implications for emergency care. *J Am Coll Emerg Physicians Open* 2020.
- [4] D. Amin, N. Nguyen, S.M. Roser, S. Abramowicz, 3D Printing of Face Shields During COVID-19 Pandemic: A Technical Note, *Journal of Oral and Maxillofacial Surgery* In press, corrected proof Available online May 1 2020,
- [5] B.I. Oladapo, S.A. Zahedi, S. Chong, F.T. Omigbodun, I.O. Malachi, 3D printing of surface characterisation and finite element analysis improvement of PEEK-HAP-GO in bone implant, *Int. J. Adv. Manuf. Tech.* 106 (2020) 829-841.
- [6] S. Ishack, S.R. Lipner, Applications of 3D Printing Technology to Address COVID-19–Related Supply Shortages, *Amer. J. Med.*, In press, corrected proof Available online April 21 2020.
- [7] L. Maracaja, D. Blitz, D.L.V. Maracaja, C.A. Walker, How 3D Printing Can Prevent Spread of COVID-19 Among Healthcare Professionals During Times of Critical Shortage of Protective Personal Equipment, *Journal of Cardiothoracic and Vascular Anesthesia* In press, corrected proof Available online April 13 2020.

- [8] B. Naik, N. Gupta, R. Ojha, S. Singh, D. Prusty, High throughput virtual screening reveals SARS-CoV-2 multi-target binding natural compounds to lead instant therapy for COVID-19 treatment, *International Journal of Biological Macromolecules*, Vol, 1601 (2020) 1-17.
- [9] F. Walsh, Coronavirus: mercedes F1 to make breathing aid accessed, <https://www.bbc.com/news/health-52087002> (2020), (accessed March 30, 2020).
- [10] WHO dashboard Coronavirus, accessed, <https://experience.arcgis.com/experience/685d0ace521648f8a5beec1b9125cd> (2020), (accessed April 12, 2020).
- [11] L. Maracaja, D. Blitz, D.L.V. Maracaja, C.A. Walker, How 3D Printing Can Prevent Spread of COVID-19 Among Healthcare Professionals During Times of Critical Shortage of Protective Personal Equipment, *J. Cardioth Vascul Anesth*, In press, corrected proof Available online April 13 2020.
- [12] E. Li, A. Larson, A. Kothari, M. Prakash, Handyfuge-LAMP: low-cost and electricity-free centrifugation for isothermal SARS-CoV-2 detection in saliva.doi: <https://doi.org/10.1101/2020.06.30.20143255>.
- [13] C. De, X.H. A. Rebaza, et al. Protecting healthcare workers from subclinical coronavirus infection. *Lancet Respir. Med.* (2020) 8-13.
- [14] J.F. Chan, et al. A familial cluster 2019 novel coronavirus indicating ptp transmission: A study of a family cluster. *Lancet* 395 (2020) 514–523.
- [15] J. Luo, M. Wu, D. Gopukumar, Y. Zhao, Big data application in biomedical research and health care: a literature review, *Biomed. Inf. Insights* 8 (2016) 31559, 10.4137/bii.s31559.
- [16] K. Gelles, G. Petras, How ventilators work and why COVID-19 patients need them to survive Coronavirus, USA. Today (2020), <https://www.usatoday.com/in-depth/news/2020/04/10/coronavirus-ventilator-how-works-why-covid-19-patients-need/2942996001/>, (accessed April 11, 2020).
- [17] M. Sapoval, et al, 3D-printed face protective of COVID-19 pandemic, diagnostic and interventional imaging, In press, corrected proof Available online April 18 2020.
- [18] PRAKASH LAB, Curiosity-Driven Science, COVID-19 Response, <http://web.stanford.edu/group/prakash-lab/cgi-bin/labsite/covid19/> (Assessed September 17 2020).
- [19] K. Prasad, F. Khatoon, S. Rashid, N. Ali, V. Kumar, Targeting hub genes and pathways of innate immune response in COVID-19: A network biology perspective, *Inter. J. Biol. Macromol.* 16315 (2020) 1-8.
- [20] R.M. Elavarasan, R. Pugazhendhi, Restructured society and environment: A review on potential technological strategies to control the COVID-19 pandemic, *Sci. Total Env.* 72510 (2020) 138858.
- [21] M. Acuto, COVID-19: Lessons for an Urban(izing) World, *One Earth* 2 (2020) 317-319.
- [22] B.I. Oladapo, A.O.M. Adeoye., M. Ismail, Analytical optimization of a nanoparticle of microstructural fused deposition of resins for additive manuf, *Compos. Part B Eng.* 150 (2018) 248-254.
- [23] N. Zhu, D. Zhang, W. Wang, X. Li, B. Yang, J. Song, et al., A novel coronavirus from patients with pneumonia in China, *N Engl J Med* (2019) 382, 10.1056/NEJMoa2001017.

- [24] 3Dnatives, Medically approved emergency 3D-printed ventilator goes into production, accessed, <https://www.3dnatives.com/en/3d-printed-respirator-230320205/> (2020), (accessed March 23, 2020).
- [25] R. Gupta, A. Ghosh, A.K. Singh, A. Misra, Clinical considerations for patients with diabetes in times of COVID-19 epidemic. *Diabetes & Metabolic Syndrome, Clin. Res. Rev.* 14 (3) (2020) 211-212.
- [26] European Centre for Disease Prevention and Control, An agency of the European Union, <https://www.ecdc.europa.eu/en/geographical-distribution-2019-ncov-cases> (sept. 14 2020).
- [27] U. Pua, D. Wong, What is needed to make interventional radiology ready for COVID-19? Lessons learned from SARS-Cov epidemic, *Korean J. Radiol.* (2020) 10.3348/kjr. 2020.0163.
- [28] G.R.J. Swennen, L. Pottel, P.E. Haers, Custom-made 3D-printed available FFP2/3 masks, *Inter. J. Oral Maxillofac. Surg.* 49 (2020) 673-677.
- [29] S.T. Flanagan, D.H. Ballard, 3D-printed Face Shields: A Community Response to the COVID-19 Global Pandemic, *Academic Radiology* In press, corrected proof Available online April 17 2020.
- [30] S. Sanami, M. Zandi, B. Pourhossein, G-R. Mobini, M. Alizadeh, Design of a multi-epitope vaccine against SARS-CoV-2 using immunoinformatics approach, *Inter. J. Biological Macromol.*, In press, journal pre-proof Available online July 15 2020.
- [31] J. Sarkis, M.J. Cohen, P. Dewick, P. Schröder, A brave new world: Lessons from the COVID-19 pandemic for transitioning to sustainable supply and production, *Res. Cons. Recycl.* 159 (2020) 104894..
- [32] V. Palmieri, M. Papi, Can graphene take part in the fight against COVID-19?, *Nano Today* 33 (2020) 100883.
- [33] B.I. Oladapo, I.A. Daniyan, O.M. Ikumapayi, O.B. Malachi, I.O. Malachi, Microanalysis of hybrid characterization of PLA/cHA polymer scaffolds for bone regeneration, *Polym. Test.* 83 (2020) 106341.
- [34] R. Vaishya, A. Haleem, A. Vaish, M. Javaid, Emerging Technologies to combat the COVID-19 pandemic, *J. Clin. Experim. Hepatol.* In press, corrected proof Available online May 5 2020.
- [35] S. Wellman, J. Moskal, C. L. Barnes, J. Parvizi, Business unusual: COVID-19 ramifications for arthroplasty, *J. Arthroplas* In press, corrected proof Available online April 24 2020.
- [36] R. Gupta, A. Misra, Contentious issues and evolving concepts in the clinical presentation and management of patients with COVID-19 infection with reference to use of therapeutic and other drugs used in Co-morbid diseases (hypertension, diabetes, etc). *Diabetes & metabolic syndrome, Clin. Res. Rev.* 14 (2020) 251-254.
- [37] How India's fighting COVID with low cost ventilators and face shields, *The Times of India* (April 4 2020), <https://timesofindia.indiatimes.com/india/how-indias-fighting-covid-19-with-low-cost-ventilators-face-shields/articleshow/74962863.cms>.
- [38] B.I. Oladapo, A.A. Victor, I.E. Elemure, Microstructural 4D printing investigation of ultra-sonication biocomposite polymer. *J. King Saud. Univ. Eng. Sci.* (2019) 1-7.
- [39] J.L. Penarredonda, Covid-19: the race to build coronavirus ventilators, <https://www.bbc.com/future/article/20200401-covid-19-the-race-to-build-coronavirus-ventilators> (2020), (accessed April 1, 2020).

- [40] Coronavirus, President von der Leyen and Commissioner Breton discuss solutions with industry to ramp up production of products needed to tackle the crisis, EU Comm Press (2020), <https://www.pubaffairsbruxelles.eu/coronavirus-president-von-der-leyen-and-commissioner-breton-discuss-solutions-with-industry-to-ramp-up-production-of-products-needed-to-tackle-the-crisis-eu-commission-press/>
- [41] Allocating ventilators in a pandemic, <https://healthmanagement.org/c/icu/news/allocating-ventilators-in-a-pandemic> (2020), (accessed March 24, 2020).
- [42] G. Gabutti, E. d'Anchera, F. Sandri, M. Savio, A. Stefanati, Coronavirus: update related to the current outbreak of COVID-19, *Infect. Dis. Ther.* 8 (2020) 1-13.
- [43] MIT Technology Review, 2020a, MIT Technology Review, AI. Could Help with the Next Pandemic - But Not with this One, <https://www.technologyreview.com/2020/03/12/905352/ai-could-help-with-the-next-pandemic-but-not-with-this-one/> (2020), (accessed March 17, 2020).
- [44] ITN, Dutch companies offer free innovative COVID-19 AI software, <https://www.itnonline.com/content/dutch-companies-offer-free-innovative-covid-19-ai-software> (2020).
- [45] Klaviyo, Key trends in brands, <https://www.klaviyo.com/covid-19-ecommerce-marketing-poll> (2020), (accessed March 28, 2020).
- [46] V.A. Balogun, B.I. Oladapo, Electrical energy demand modeling of 3D printing technology for sustainable manufacture, *Int. J. Eng.* 29 (2016) 954-961.
- [47] C-C. Lai, T-P. Shih, W-C. Ko, H-J. Tang, P-R. Hsueh, Severe acute respiratory syndrome coronavirus 2 (SARS-CoV-2) and corona virus disease-2019 (COVID-19): the epidemic and the challenges, *Int. J. Antimicrob. Agents*, 55 (2020) 105924, 10.1016/j.ijantimicag.2020.105924.
- [48] M. Wang, T. Fu, J. Hao, L. Li, C. Li, A recombinant *Lactobacillus plantarum* strain expressing the spike protein of SARS-CoV-2, *Inter. Biol. Macromol.* 1601 (2020) 736-740.
- [49] NS Medical Devices, Manufacturing of key medical kit during COVID-19, <https://www.nsmedicaldevices.com/analysis/companies-ventilators-shortage-coronavirus/> (2020), accessed April 2, 2020.
- [50] Y. Lei, B. Yang, X. Jiang, F. Jia, et al., Applications of machine learning to machine fault diagnosis: a review and roadmap, *Mech. Syst. Signal Process.* 138 (2020)106587, 10.1016/j.ymssp.2019.106587.
- [51] MIT, Technology Review, Over 24,000 Coronavirus Research Papers Are Now Available in One Place, <https://www.technologyreview.com/2020/03/16/905290/coronavirus-24000-research-papers-available-open-data/> (2020), (accessed March 21, 2020).
- [52] J.C. Rosser, V. Vignesh, B.A. Terwilliger, B.C. Parker, Surgical and medical applications of drones: A comprehensive review, *J. Soc. Laparoendos Surg.* 22 (2018) 2018.00018, 10.4293/jsls.2018.00018.
- [53] B.I. Oladapo., S.O. Ismail, M. Zahedi, A. Khan, H. Usman, 3D printing and morphological characterisation of polymeric composite scaffolds, *Eng. Struct.* 216 (2020) 110752.

- [54] Z. Zehra, M. Luthra, S. M. Siddiqui, A. Shamsi, A. Islam, Corona virus versus existence of human on the earth: A computational and biophysical approach, *Inter. J. Biol. Macromol.* 16115 (2020) 271-281.
- [55] N. van Doremalen, T. Bushmaker, D.H. Morris, M.G. Holbrook, A. Gamble, B.N. Williamson, et al., Aerosol and surface stability of SARS-CoV-2 as compared with SARS-CoV-1, *N. Engl. J. Med.* 382 (2020) 1564-1567.
- [56] The Economic Times, Robots help combat COVID-19 in world, and maybe soon in India too, <https://economictimes.indiatimes.com/news/science/robots-help-combat-covid-19-in-world-and-maybe-soon-in-india-too/articleshow/74893405.cms> (2020), (accessed April 1, 2020).
- [57] J.J. Van Bavel, et al., Using support COVID-19 pandemic response, *PsyArXiv preprints* (2020), 10.31234/osf.io/y38m9.
- [58] B.I. Oladapo, E.A. Oshin, A.M. Olawumi, Nanostructural computation of 4D printing carboxymethylcellulose (CMC) composite. *Nano-Struct Nano-Obj.* 21 (2020) 100423.
- [59] Verdict Medical devices, Screening for COVID-19, <https://www.medicaldevice-network.com/features/types-of-covid-19-test-antibody-pcr-antigen/> (2020), (accessed April 4, 2020).
- [60] L. Wang, J. Li, S. Guo, N. Xie, Real-time estimation and prediction of mortality caused by COVID-19 with patient information-based algorithm, *Sci. Total Environ.* (2020), 10.1016/j.scitotenv.2020.138394.
- [61] D. Ben-Israel, W.B. Jacobs, S. Casha, S. Lang, W.H.A. Ryu, et al., The impact of machine learning on patient care: A systematic review, *Artif. Intell. Med.*, 103 (2019) 101785, 10.1016/j.artmed.2019.101785.
- [62] H. Jiang, Y. Sheng, T. Ngai, Pickering emulsions: Versatility of colloidal particles and recent applications, *Curr. Opin. Coll. Interf. Sci.* 49 (2020) 1-15.
- [63] EdTechReview, 2020, EdTechReview, Countries Which Are Leading the Way in Online Education, <https://edtechreview.in/e-learning/3028-countries-leading-in-online-education> (2020), accessed March 22, 2020.
- [64] R. Kellermann, T. Biehle, L. Fischer, Drones for parcel and passenger transportation: A literature review, *Transport. Res. Inter. Persp.* (2020) 100088, 10.1016/j.trip.2019.100088.
- [65] S.P.L. Kumar, State of the art-intense review on artificial intelligence systems application in process planning and manufacturing, *Eng. Appl. Artif. Intell.*, 65 (2017) 294-329, 10.1016/j.engappai.2017.08.005.
- [66] S. Gondi, A.L. Beckman, N. Deveau, A.S. Raja, S. He, Personal protective equipment needs in the USA during the COVID-19 pandemic, *Lancet* 395 (2020) 90-91.
- [67] B. I. Oladapo, S.A. Zahedi, F. Vahidnia, O.M. Ikumapayi, M.U. Farooq, Three-dimensional finite element analysis of a porcelain crowned tooth, *Beni-Suef Univ. J. Basic Appl. Sci.* 7 (2018) 461-464.
- [68] CIO, 2020, How the COVID-19 pandemic is reshaping healthcare with technology. <https://www.cio.com/article/3534499/how-the-covid-19-pandemic-is-reshaping-healthcare-with-technology.html> (accessed March 29, 2020).
- [69] EdTechReview, Countries Which Are Leading the Way in Online Education, <https://edtechreview.in/e-learning/3028-countries-leading-in-online-education> (2020), (ccessed March 22, 2020).

- [70] Financial Express, Tech-Ing on Covid-19, <https://www.financialexpress.com/opinion/tech-ing-on-covid-19-govt-must-extensively-use-tech-solutions-to-fight-coronavirus/1909609/> (2020), (ccessed March 28, 2020).
- [71] E. Cesewski, B.N. Johnson, Electrochemical biosensors for pathogen detection, *Biosens. Bioelect.* 1591 (2020) 112214.
- [72] Enforcement policy for face masks and respirators during the coronavirus disease (COVID-19) public health emergency staff. Food and Drug Administration Website. Available at: <https://www.fda.gov/media/136449/download>, (accessed April 6, 2020).
- [73] India Today, Rapid antibody tests, [https://www.medicaldevice-network.com/features/types-of-covid-19-test-antibody-pcr-antigen/\(2020\)](https://www.medicaldevice-network.com/features/types-of-covid-19-test-antibody-pcr-antigen/(2020)), (accessed April 5, 2020).
- [74] ITN, Two Studies Use SIRD Model to Forecast COVID-19 Spread, <https://www.itnonline.com/content/two-studies-use-sird-model-forecast-covid-19-spread> (2020).
- [75] S. Ratzan, L. Gostin, N. Meshkati, K. Rabin, R. Parker, COVID-19: NAM Perspectives. Commentary, National Academy of Medicine, Washington, DC (2020), 10.31478/202003a.
- [76] Techcrunch, Dyson and Gtech support for COVID-19, <https://techcrunch.com/2020/03/26/dyson-and-gtech-answer-uk-call-for-ventilator-design-and-production-to-support-covid-19-response/?guccounter=1> (2020), (accessed March 29, 2020).
- [77] World Health Organization, Coronavirus disease (COVID-19) advice for the public: when and how to use masks, WHO (2020), <https://www.who.int/emergencies/diseases/novel-coronavirus-2019/advice-for-public/when-and-how-to-use-masks>, (accessed March 17, 2020).
- [78] M.L. Ranney, V. Griffeth, A.K. Jha, Critical during the COVID-19 pandemic, *N. Engl. J. Med.* (2020), 10.1056/NEJMp2006141.
- [79] World Economic Forum, Innovation in meeting the ventilator demands, <https://www.weforum.org/agenda/2020/03/coronavirus-ventilators-covid19-healthcare/> (2020).
- [80] WHO, The COVID-19 Risk Communication Package for Healthcare Facilities, <https://iris.wpro.who.int/bitstream/handle/10665.1/14482/COVID-19-022020.pdf> (2020), (accessed March 20, 2020).
- [81] K. Chon Ng Kee Kwong, Puja R. Mehta, Garima Shukla, Arpan R. Mehta, COVID-19, SARS and MERS: A neurological perspective, *J. Clin. Neurosci.* In press, corrected proof Available online May 5 2020.
- [82] Y. Jin, H Yang, W Ji, W Wu, S Chen, W Zhang, et al., Virology, epidemiology, pathogenesis, and control of COVID-19, *Viruses*, 12 (2020) 372.
- [83] F. Jiang, L. Deng, L. Zhang, Y. Cai, C.W. Cheung, Z. Xia, Review of the clinical characteristics of coronavirus disease 2019 (COVID-19), *J. Gen. Intern. Med.* 35 (2020) 1545-1549.
- [84] S. Tian, W. Hu, L. Niu, H. Liu, H. Xu, S.Y. Xiao, Pulmonary pathology of early-phase 2019 novel coronavirus (COVID-19) pneumonia in two patients with lung cancer, *J. Thorac. Oncol.* 15 (2020), 700-704.

- [85] M. Sachdeva, R. Gianotti, M. Shah, B. Lucia, R.P. Dodiuk-Gad, Cutaneous manifestations of COVID-19: Report of three cases and a review of literature, *J. Dermatol. Sci.* In press, corrected proof Available online April 29 2020.
- [86] B.I. Oladapo, O.B. Obisesan, O. Bowoto, A.A. Victor, U. Hazrat, K. Affan, Mechanical characterization of a polymeric scaffold for bone implant, *J. Mater. Sci.* 55 (2020) 9057-9069.
- [87] L-L. Yang, T. Yang, Pulmonary rehabilitation for patients with coronavirus disease 2019 (COVID-19), *Chron. Dis. Translat. Med.* In press, corrected proof Available online May 14 2020.
- [88] F. Zhou, T. Yu, R. Du, et al., Clinical course and risk factors for mortality of adult inpatients with COVID-19 in Wuhan, China: A retrospective cohort study, *Lancet* 395 (2020) 1054-1062.
- [89] Q. Ruan, K. Yang, W. Wang, L. Jiang, J. Song, Clinical predictors of mortality due to COVID-19 based on an analysis of data of 150 patients from Wuhan, China, *Intens. Care Med.* 46 (2020) 846-848.
- [90] F.A. Klok, MJHA Kruij, N.J.M. van der Meer, et al., Incidence of thrombotic complications in critically ill ICU patients with COVID-19, *Thromb Res.* S0049-3848 (2020) 30120-30121.
- [91] P. Zhai, Y. Ding, X. Wu, J. Long, Y. Zhong, Y. Li, The epidemiology, diagnosis and treatment of COVID-19, *Int. J. Antimicrob. Agents*, 28 (2020) 105955.
- [92] B.I. Oladapo, S.A. Zahedi, A.O.M. Adeoye, 3D printing of bone scaffolds with hybrid biomaterials. *Compos. Part B Eng.* 158 (2019) 428-436.
- [93] I.F. Manalo, M.K. Smith, J. Cheeley, R. Jacobs, A dermatologic manifestation of COVID-19: transient livedo reticularis, *J. Am. Acad. Dermatol.* 83 (2020) 700.
- [94] B. Joob, V. Wiwanitkit, COVID-19 can present with a rash and be mistaken for dengue, *J. Am. Acad. Dermatol.* 82 (2020) 177.
- [95] A. Alramthan, W. Aldaraji, A case of COVID-19 presenting in clinical picture resembling chilblains disease. First report from the Middle East, *Clin. Exp. Dermatol.* (2020).
- [96] A. Kolivras, F. Dehavay, D. Delplace, F. Feoli, I. Meiers, L. Milone, et al., Coronavirus (COVID-19) infection-induced chilblains: a case report with histopathological findings, *JAAD Case Rep.* (April 18) (2020).
- [97] F. Zhou, T. Yu, R. Du, et al., Clinical course and risk factors for mortality of adult inpatients with COVID-19 in Wuhan, China: A retrospective cohort study, *Lancet* 395 (2020), 1054-1062.
- [98] Y.R. Guo, Q.D. Cao, Z.S. Hong, Y.Y. Tan, S.D. Chen, H.J. Jin, K.S. Tan, D.Y. Wang, Y. Yan, The origin, transmission and clinical therapies on coronavirus disease 2019 (COVID-19) outbreak—An update on the status, *Mil. Med. Res.* 13 (2020) 11.
- [99] S. El Hayek, M.A. Cheaito, M. Nofal, D. Abdelrahman, H. Al Sinawi, Geriatric mental health and COVID-19: An eye-opener to the situation of the Arab countries in the Middle East and North Africa Region, *Amer. J. Geriatric Psych.* In press, Journal Pre-proof Available online May 18 2020.
- [100] İ. Devrim, N. Bayram, Infection control practices in children during COVID-19 pandemic: differences from adults, *Amer. J. Infect. Cont.* In press, Journal Pre-proof Available online May 26 2020.

- [101] C.F. Tam, K.S. Cheung, S. Lam, et al., Impact of coronavirus disease 2019 (COVID-19) outbreak on ST-segment-elevation myocardial infarction care in Hong Kong, China, *Circ. Cardiovasc. Qual. Outcomes* 13 (2020) 006631.
- [102] J. Rodriguez-Pardo, B. Fuentes, M.A. de Leciñana, J. Campollo, P.C. Castaño, J.C. Ruiz, et al., Atención al ictus agudo durante la pandemia por COVID-19, *Recomendaciones Plan Ictus Madrid, Neurologia* (2020).
- [103] Z. Xu, L. Shi, Y. Wang, et al., Pathological findings of COVID-19 associated with acute respiratory distress syndrome, *Lancet Respir. Med.* 8 (2020) 420-422.
- [104] G.M. Paul, A. Rezaenia, P. Wen, S. Condoor, N. Parkar, W. King, T. Korakiantis, Medical applications for 3D printing: Recent developments, *Mo. Med.* 115 (1) (2018) 75-81.
- [105] C. Li, D. Pisignano, Y. Zhao, J. Xue, Advances in medical applications of additive manufacturing, *Engineering* 2020, <https://doi.org/10.1016/j.eng.2020.02.018>.
- [106] O. Hooper, Five ethical concerns with 3D printing in medicine. *Law technology today*, <https://www.lawtechnologytoday.org/2020/05/five-ethical-concerns-with-3d-printing-in-medicine/> (accessed October 17, 2020).
- [107] Deloitte, 3D opportunity for health care: Demystifying FDA regulations for medical devices, 2017, <https://www2.deloitte.com/us/en/insights/focus/3d-opportunity/additive-manufacturing-fda-regulations-medical-devices.html#> (accessed October 17, 2020).
- [108] M.J. Walker, Ethics and advanced medical devices: Do we need a new approach? *J. Cons. Health Forum Australia* 2020.
- [109] F. Gilbert, C.D. O'Connell, T. Mladenovska, S. Dodds, Print me an organ? Ethical and regulatory issues emerging from 3D bioprinting in medicine, *Sci. Eng. Ethics* 24 (2018) 73-91.
- [110] M. Kritikos, 3D bio-printing for medical and enhancement purposes: Legal and ethical aspects. *European Parliamentary Research Service (EPRS)*, 2018, [https://www.europarl.europa.eu/RegData/etudes/IDAN/2018/614571/EPRS\\_IDA\(2018\)614571\(ANN2\)\\_EN.pdf](https://www.europarl.europa.eu/RegData/etudes/IDAN/2018/614571/EPRS_IDA(2018)614571(ANN2)_EN.pdf) (accessed October 17, 2020).